



NEVADA DIVISION OF  
**ENVIRONMENTAL  
PROTECTION**

**STATE OF NEVADA**  
Department of Conservation & Natural Resources

Brian Sandoval, Governor  
Leo M. Drozdoff, P.E., Director  
David Emme, Administrator

July 25, 2016

Phigenics Analytical Services Laboratory  
1701 Quincy Ave., Suite 32  
Naperville, IL 60540

EPA ID# IL01240

RE: Nevada Environmental Laboratory Certification 1 Year Extension.

Dear Sir or Madam:

Your laboratory's 2015-2016 Nevada scope has been extended until July 31, 2017 or until you receive the updated 2016-2017 scope.

This will serve as official notice to you and your clients.

**Be advised this letter is only valid as long as your laboratory maintains compliance with State of Nevada regulation NAC 445A.0552 to .067, NAC 445A.542 to .54296 and/or NAC 459.96902 to .9699.**

Failure to do so will result in invalidation of any data submitted to the Nevada Department of Environmental Protection.

If you or your clients have any questions, please contact Donald LaFara at 775-687-9491.

Sincerely,

Donald LaFara, Laboratory Certification Officer  
Branch Supervisor, Laboratory Certification Program  
State of Nevada Division of Environmental Protection

**State of Nevada Department of Conservation and Natural Resources  
Division of Environmental Protection  
Laboratory Scope of Accreditation**

**EPA Number: IL01240**


**Attachment to Certificate Number: IL012402017-1**

**Expiration Date: 7/31/2017**

Phigenics Analytical Services Laboratory  
1701 Quincy Ave., Suite 32 Naperville, IL 60540

**Matrix: SDWA (Potable Water)**

Method	Analyte	Start Date	Date Expires	Status
Discipline Microbiology				
Modified Colitag	Escherichia coli	8/1/2016	7/31/2017	Certified
Modified Colitag	Total coliforms	8/1/2016	7/31/2017	Certified
SM 9215 B (PCA)	Heterotrophic plate count	8/1/2016	7/31/2017	Certified

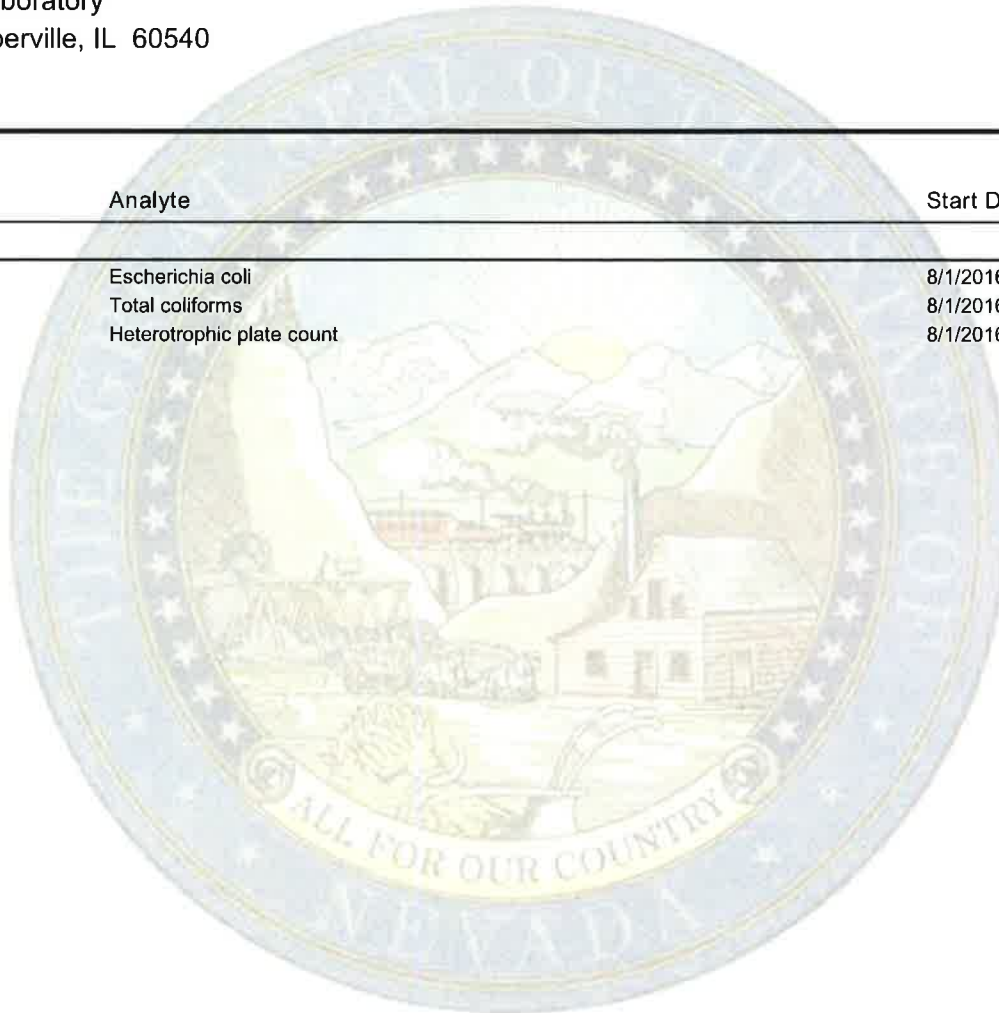

**Disclaimer: A laboratory that is certified or approved has established that they have the ability to implement a quality control program in accordance with the appropriate Federal or State regulations or statutes. It is the certified laboratory's responsibility to provide their client the most current certified parameter list. Contact LCP to verify certification status.**